


reproducibility test: Andrews et al (2015)

oks00TR3-MNS-MAXX-03-01_02: sample thickness measured before and after soaking it in saline for an hour.
t1= 2.606, t2=3.028.

Protocol:

- a) 1g load with 0.005 mm/s, wait for 10 mins,
- b) 2% strain of t2 at 0.5mm/s , wait for an hour,
- c) recompress to t1 (0.422 mm) at 0.0005 mm/s, wait for 5000s,
- d) 2% strain of t1 at 0.5mm/s,wait for 1hr,
- e) unload by -4mm.
- f) Confined compression test
- g) Behavior in agreement with the study predictions.

b)

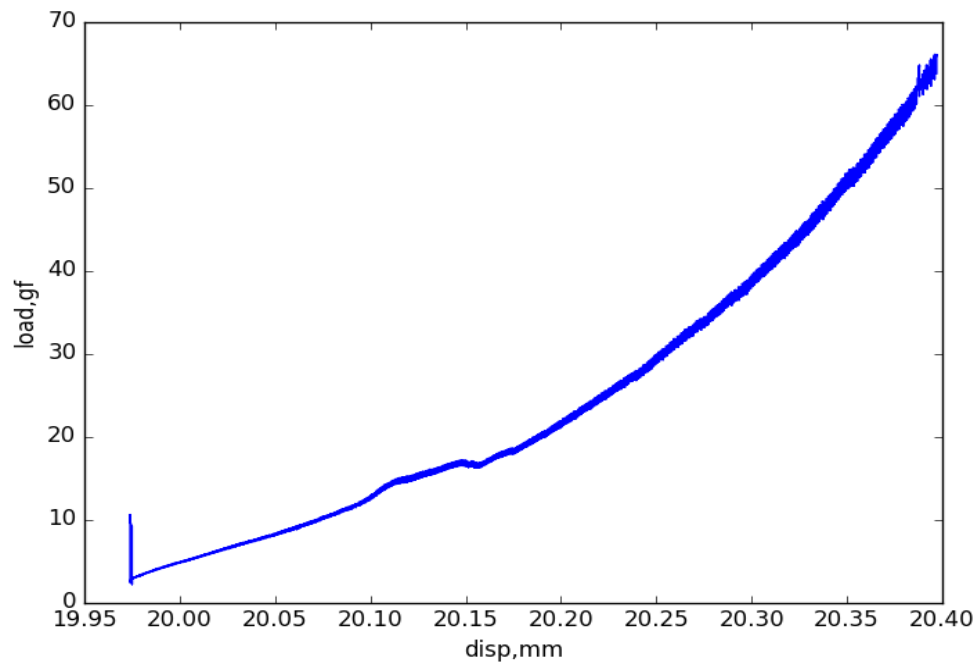

d)

